

User manual

meywalk[®] 4

Model Mini, Small, Medium and Large



CE

meyland-smith
mobility and more

Contents

Introduction.....	3
CE marking and labels.....	3
Safety precautions.....	3
Prior to first use.....	4
Meywalk® 4 parts.....	4
Joining the top part and bottom frame.....	5
Spring loading.....	5
Adjustment / step by step	6
Tubes.....	6
Handlebar.....	6
Seat.....	7
Trunk support height.....	7
Trunk support replacement.....	7
Tilt function.....	8
Getting in and out.....	8
Rear stop.....	8
Trunk support.....	9
Brakes.....	9
Drag brakes.....	9
Non/reverse brakes.....	9
Front wheel swivel/locks.....	9
Accessories.....	10
Antitip supports.....	10
Leg divider.....	10
Leg guide.....	10
Trunk pad.....	11
Hip pads.....	11
Cleaning, disinfection and maintenance.....	11
Recycling.....	11
Disposal	11
Warranty.....	12

Introduction

Meywalk® 4 Mini, Small, Medium and Large are primarily designed for walking -disabled children, youths and adults who have difficulty standing up without support. The user-friendly Meywalk® 4 is designed for indoor use. The maximum body weight of the user permitted to Mini is 50 kg, to Small is 100 kg and to Medium and Large are 130 kg.

With the Meywalk® 4 you have purchased one of the best walkers available. A higher standard is reached due to its unique design and high-quality materials. You will be impressed by the multiple functions:

- :: Meywalk® 4 follows individual body movements and walking patterns.
- :: Helps the user keep his/her torso upright and makes the user feel safe.
- :: The handlebar supports the user's arms and reduces the strain on them.
- :: The seat can be lowered when getting in and out.
- :: The rear stop helps with keeping the user comfortably seated.
- :: The integrated springs and dynamic seat support the walking function.

CE marking and labels

The type and manufacturer label is placed on the bottom frame. Labels must always be readable. Replace any unreadable or missing labels as soon as possible. The type and manufacturer label is important for the identification of the product and may not be removed.

The Meywalk® 4 is CE marked. This guarantees that the Meywalk® 4 is in compliance with all relevant safety requirements specified in Council Directive 93/42/EEC on medical devices. The Meywalk® 4 was tested by Berlin Cert, Prüf- und Zertifizierstelle für Medizinprodukte GmbH, at the Berlin Technical University.

Safety precautions

Never leave the user in Meywalk® 4 unattended! Meywalk® 4 is a therapy product and should only be used as such!

The spring system of Meywalk® 4 may involve a risk of the walking aid toppling over if used by a very restless user.

Meywalk® 4 rolls very easily and you should always consider potential dangers that the user may roll over to.

Always hold the tilt bar securely when a user is being lifted or lowered. Especially when opening the tilt bar to lower the user, you must be prepared for the upward force which gradually increases as the tilt bar rises. Never let go of the tilt bar in the middle of a lifting or lowering operation, even if taken by surprise by the heavy weight loading.

Be aware of the higher risk of squeezing your fingers when adjusting the walker.

If fittings are removed, open tube ends may be revealed. These may have sharp inner edges and may be dangerous for probing fingers. However, Meywalk® 4 and its

accessories are designed to avoid

open ends! If a situation with open tube ends should nevertheless arise, it is recommended that they be closed off with plastic plugs.

Polyurethane foam and foam tubing may not be consumed.

Please be aware that the upholstery heats up if placed in direct sun light. This can cause skin damage if the upholstery is touched. Therefore, cover up the upholstery parts or protect the walker from direct sun light.

The walker should only be used on level and firm flooring. Avoid loose surfaces such as gravel, sand or foliage. Be aware of unevenness's and holes in the flooring as there is a risk of toppling over or getting stuck.

Be especially careful on wet or icy surfaces as the risk of slipping is considerably higher. Please check that all parts are securely fastened before using the walker. Do not use high-pressure cleaning tools or caustic chemicals when cleaning the walker.

Unlike previous generations of Meywalk® Walkers is the Meywalk® 4 now equipped with drag brakes, non-reverse brakes and front wheel swivellocks as standard.

Prior to first use

Meywalk® 4 is supplied almost fully assembled. Check that the package contains the following parts:

- :: Bottom frame with wheels and brakes.
- :: Top part with seat and trunk support.
- :: A set of springs according to the user's body weight.
- :: Accessories as ordered.

Meywalk® 4 Parts



Joining the top part and bottom frame:

Place the top part in the tubes on the bottom frame. Remember to position the top part so that the handlebar points in the direction of the swivelling front wheels.



Spring loading

The two springs inside the tubes can be changed to obtain harder or softer suspension. As a guideline, the springs should be fully compressed by the body weight of the user. There are seven different spring hardness levels corresponding to the following body weight:



Mini:

:: Orange springs for 10 -15 kg.

:: Purple springs for 15 - 20 kg.

Mini and Small:

:: White springs for 20 - 50 kg.

Small, Medium and Large:

:: Yellow springs for 45 - 65 kg.

:: Blue springs for 65 - 80 kg.


Medium and Large:

:: Red springs for 80 - 100 kg.

:: Silver springs for 100 - 130 kg.

The springs can easily be interchanged. Grab and open the swing bar so that the frame is lowered. The tube ends are closed with a lid - open the lids to remove the springs. To open the lid push up and turn clockwise before pulling the lid down and off. After removal of the old springs the new ones can be inserted into the tubes. Now the lid can be fastened again by repeating the steps above in reverse order.

On the Model Mini, you have to lift the top part, then you can easily change the springs.

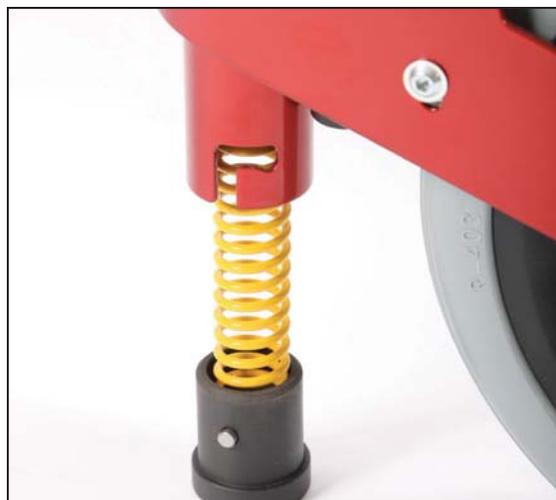

Adjustments — step by step

It is always a good idea to consult one of our professionals before adjustment of Meywalk® 4.

Stanchions

Warning! Do not carry out this adjustment while a user is placed in Meywalk® 4.

The height of Meywalk® 4 is adjusted by way of the black spanner grips. Loosen the spanner grips on both sides and adjust the frame to the desired height. Fasten the spanner grips firmly. It is important that both sides are adjusted to an equal height. You can check this by way of the indentations on the tubes.




Handlebar

The angle of the handlebar can be adjusted in three steps. Loosen the two thumb screws and turn the handlebar to the desired position.

Fasten the thumb screws lightly. If the handlebar is seated correctly it should not be possible to turn it with the thumb screws lightly fastened.

When you have made sure that the handlebar is placed correctly you may tightly fasten the thumb screws.


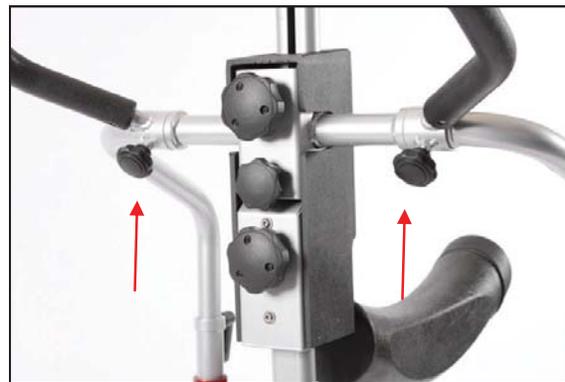


Seat

Warning! Do not carry out this adjustment while a user is placed in Meywalk® 4.

Adjust the seat height according to the length of the user's legs. Turn the lower thumb screw located at the front of Meywalk® 4. The thumb screw features a "child lock" which is released by simultaneously pressing and turning. When released, the seat can be adjusted up or down. Position the seat at the correct height. Hold your hand under the seat bar bottom to make the seat slide easily up and down.

Re-tighten the thumb screw when the desired height has been found.

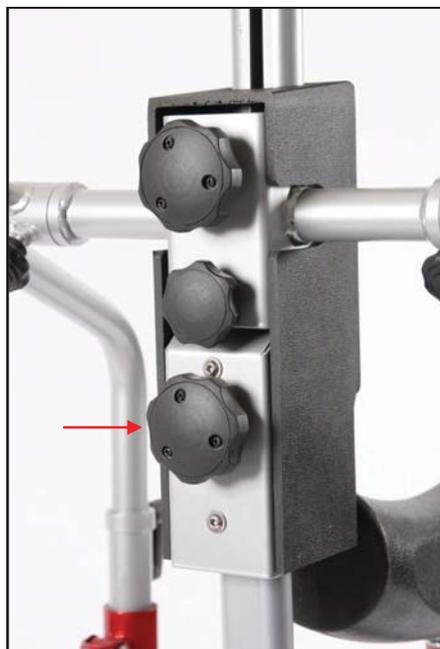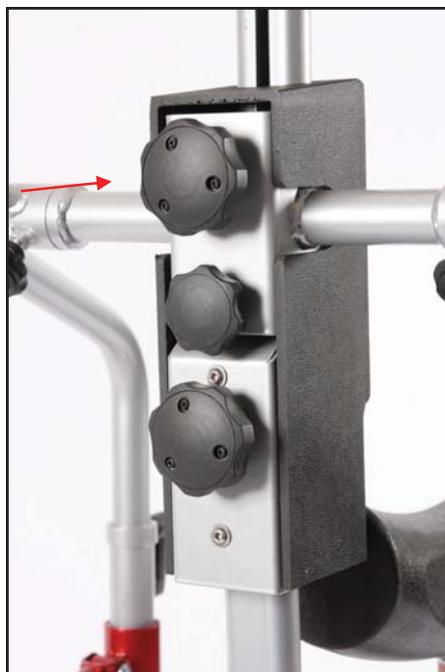

Trunk support height

Adjust the trunk support according to the individual user's height. Turn the upper thumb screw located at the front of Meywalk® 4. The thumb screw features a "child lock" which is released by simultaneously pressing and turning. When released, the trunk support can be adjusted up or down until the correct height has been found. Re-tighten the thumb screw.

Trunk support replacement

Warning! Do not carry out this adjustment while a user is placed in Meywalk® 4.

For trunk support replacement, loosen the two Allen screws in front of the support. The two screws fit all trunk supports.

The trunk support is available in five variants:


Circumference 70, 90, 105, 120 and 130 cm.



Tilt function

Warning! Do not carry out this adjustment while a user is placed in Meywalk® 4.

By means of the tilt function the user's posture can be changed. Turn the middle thumb screw to tilt the support. The thumb screw is located at the front of Meywalk® 4. While turning the screw, you can change the angle of the trunk support and seat up to 15°. The tilt function is continuously adjustable.

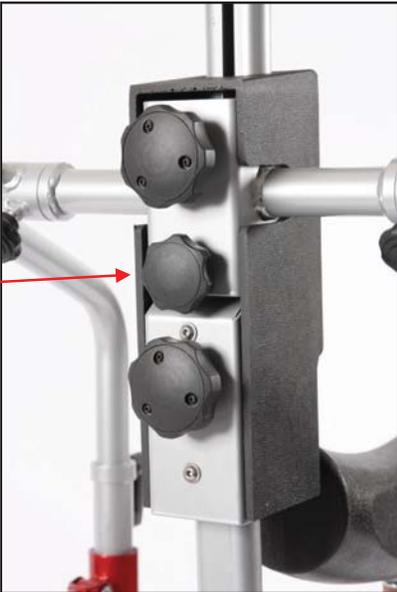

Getting in and out

Featuring a unique lifting and lowering system Meywalk® 4 has made it easier for the user to get in and out. Grab the front of the swing bar with both hands and tip it up. This way the seat will be lowered approx. 11 cm for Small, 13 cm for Medium and 22 cm for Large. When the user has been seated, close the trunk support and pull up the rear stop. The seat is lifted by pushing down the swing bar until it locks with an audible click. The integrated gearing in the lifting and lowering system means that the downward pressure need only be about one third of the user's weight



Rear stop

The rear stop should always be closed in the upright position when there is a user in Meywalk® 4. Pull the rear stop backwards out of the seat and turn it upwards. Now you can push it down into the locked position. Repeat the procedure in reverse order to open the rear stop again.



The rear stop behind the seat can be adjusted in depth. First lift up the rear stop and tilt it backwards. This reveals an Allen screw inside the U-profile. When the Allen screw is loosened, the rear stop can be slid forwards or backwards in the external tube. After adjustment, re-tighten the Allen screw.



Trunk support:

To open the trunk support push the two padded tube pieces inwards and turn down. To close the trunk support push the tube pieces inwards and turn up to the locked position.

**Drag brakes:**

The drag brakes work by the roller at the back pressing against the tire. First loosen the nut on the Allen screw. Then turn the Allen screw to press the roller against the tire. Tighten the nut in the opposite direction. Use a method of trial and error to find the correct pressure against the tire. Test the drag brake function.

**Non-reverse brakes:**

The non-reverse brake works by the grooved side pressing against the tire preventing the wheel from going backwards. The non-reverse brake can be engaged/disengaged through the snap lock on the upper side of the brake housing. Finally test the function of the non-reverse brake.

**Brakes**

The brakes are parking brakes that work by directly blocking the rear wheels with a braking pulley pressing against the tire.

To brake the walking aid, pull the brake levers all the way backwards until they come to a definite stop. In this position the brakes are self-locking. The brakes are released by pushing the brake levers forward again.

**Front wheel swivel/locks**



To activate or de-activate the swivel-locks pull and turn the pin locks 90°.



Accessories

Anti-tip support

Anti-tip supports are mounted on each side by first removing the bolts fixing the wheels. Use a 6 mm Allen key. Place the anti-tip support against the outside of the rear fork of Meywalk® 4 so that they fall into place in the two rear fork recesses. Screw bolts on both sides back on. Re-tighten firmly.

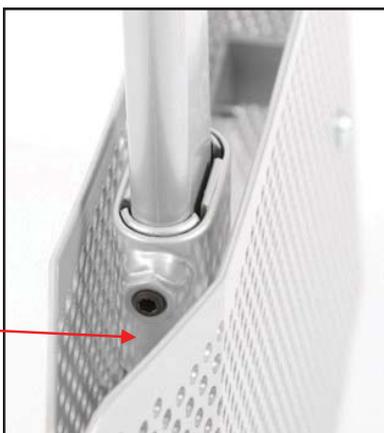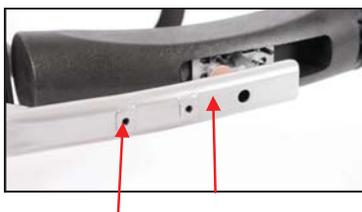

Leg divider

Fasten the leg divider under the seat bar with the two screws. The leg divider is height-adjustable. Loosen the screw at the front of the central tube. Adjust the leg divider to the desired height and re-tighten the screw firmly.

Leg guides


The leg guides are mounted on the inside of the wheel frame on either side. They are fastened at the rear fork and at the point where the connection tube is connected to the wheel frame.

Fasten the leg guides with the screws, threaded rods and Allen screw heads that came with the leg guides.



Trunk pad

The trunk pad is mounted on the black polyurethane shell of the center box. First remove the screws and washers from the shell. Then mount the trunk pad using the screws that came with the trunk pad.



Hip pads

The hip-/side pads are to be mounted on the uprights. Fit the two pipe sections around the stanchion, tighten them together using the two screws.

The hip-/side pads can be adjusted in or out of the seat by loosening the thumbscrew. Tighten the thumbscrew again after adjustment.



Height reductions set

Each reduction set consist of 1 pair of 4 units – as per below picture(1 set (1 pcs each));

- 2 pcs special fittings
- 2 pcs Threaded rod
- 2 pcs bushing
- 2 pcs Allen screw head



Loosen the tilt bar from lower frame. The existing threaded rod, the bushing and the allen screw head shall be used to mount the special fitting on the tilt bar.



The new threaded rod, the bushing and the allen screw head shall be used to mount the special fitting on the lower frame and the wide open part of the new fitting



The new threaded rod is somewhat longer than the red holder to give free access to the special fitting



NOTE

There is no Height reductions set for Mini.

Cleaning, disinfection and maintenance

Meywalk® 4 can be washed in warm water with detergent but take care not to wash the foam padding on the rear of the trunk support, handlebar and rearstop. With time the painted frame may take on a matt appearance if washed with detergent repeatedly.

If so, the frame can be polished with car polish. Follow the instructions of the polish manufacturer.

The frame and plastic parts can be disinfected with standard, alcohol-based disinfectants. The foam padding may not be disinfected.

It is recommended to regularly check the tightness of all thumbscrews, nuts, bolts and screws. Re-tighten if necessary. Check the parking brake function. When the brakes are on it should not be possible to push the walker. When the brakes are off it should be easy to push the walker. Furthermore, all moving parts should function easily and at a low level of noise. Should you experience any friction noise or squeaking, then have the walker checked by a professional.

Recycling

When handing over or recycling the walker all necessary technical documentation must be delivered to the new user to ensure safe handling. The walker must be cleaned, disinfected and checked for damages by a professional before handing over.

Disposal

When your walker is no longer in use and you wish to dispose of it please check the rules and regulations with your local waste management company.

Warranty

Warranty is granted on all defects that are proven to be caused by material or manufacturer fault. The warranty period is 24 months from the time of dispatch readiness alternatively time of delivery. The warranty does not cover any damage due to normal wear and tear, intentional, negligent or inexpedient handling or use. This also applies if using unsuitable detergents and lubricants.

Technical data	Mini	Small	Medium	Large
Length:	80 cm	85 cm	93 cm	110 cm
Outer width:	56 cm	62 cm	62 cm	68 cm
Inner width:	44 cm	49 cm	50 cm	57 cm
Seat height/inner leg length*	28-46 cm	44-67 cm	60-84 cm	80-104 cm
Trunk support height*	55-77 cm	74-99 cm	101-133 cm	120-152 cm
Trunk support circumference:	70,90,105 cm	70,90,105,120 cm	70, 90, 105, 120, 130 cm	70, 90, 105, 120, 130 cm
Weight: (without accessories):	20 kg	25 kg	32 kg	34 kg
Max load	80 kg	100 kg	130 kg	130 kg
Colours:	Yellow	Green	Red	Black
Materiale:				
Frame:	Steel tubing, powder-coated			
Fittings:	Steel powder-coated			
Upholstery:	Polyurethane			
Wheels:	Soft solid rubber tyres on plastic rims with service-free ball bearings			

*Heights are measured with half compression of springs.

Manufacturer:

Dealer:

meyland-smith
mobility and more

Meyland-Smith A/S • Mads Clausens Vej 1 • 9800 Hjørring

Phone: +45 98 96 19 85 • Fax.: +45 98 96 19 86

www.meyland-smith.dk • E-mail: info@meyland-smith.dk